

Oncology EC Film

Oncology EC Film is a high-contrast film that is coated on both sides with a very fine grain emulsion having low image noise. It is intended for radiation therapy beam localization and verification procedures. The film is designed to be used with EC-L and EC-V Lightweight Cassettes, which “sandwich” the film between a lead front screen and front and back fluorescent intensifying screens (gadolinium oxysulfide).

The film has a characteristic curve designed with the unique needs of portal imaging and verification imaging in mind. The characteristic curve (i.e., image contrast) is similar over energies from 6 to 20 MV.

The intensifying factor delivered by the use of rare-earth screens, coupled with the high-energy exposure source, allow the design of a very slow-speed, very fine-grain film emulsion. Oncology EC Film emulsion’s extremely small grain size, narrow grain size distribution, and low diffuse density variations work together to provide a very high-contrast, low-noise image. As a result, the images show clear definition of body structures, thus providing more anatomical detail.


Sensitometric and Photographic Properties:

Usage	Lightweight Cassette and/or Screen
Localization	EC-L Slow
	EC-L Regular
	EC-L Fast
Verification	EC-V Regular
	EC-V Fast

Sensitometric Parameters:

Speed	Measured at 1.0 OD above Gross Fog
Contrast	Measured as slope of the straight line portion of the sensitometric curve, and computed as the value for the rise for any three consecutive steps.
Gross Fog	Density of film base plus processing fog.

Oncology EC Film
 Simulated Green Screen Exposure; 90-second Processing
 RP X-OMAT Processor, Model M6; RP X-OMAT Chemicals; Diffuse Visual Densitometry

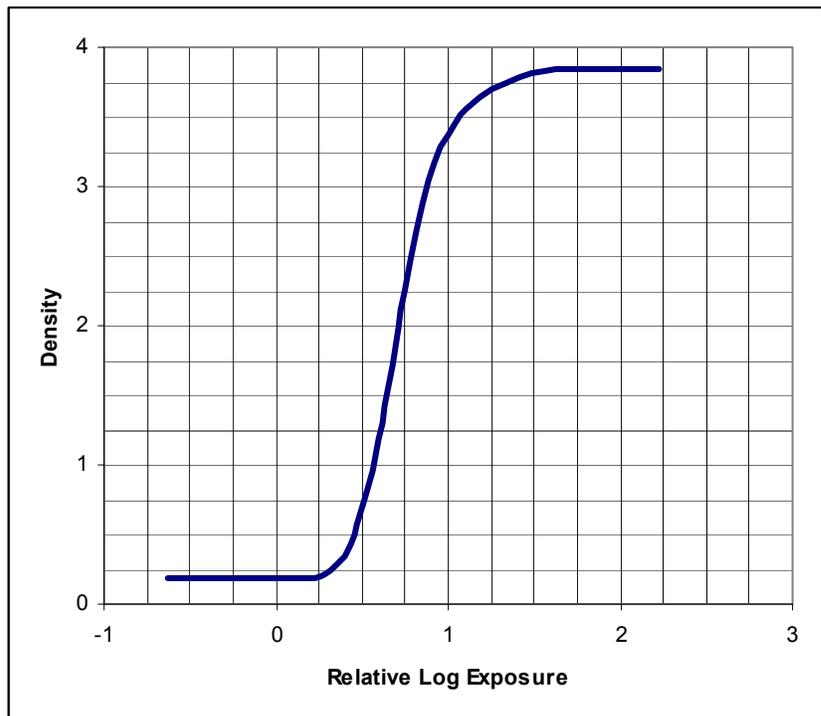

Notice: The data in this publication represent product tested under the conditions of exposure and processing specified. They are representative of production coatings, and therefore do not apply to a particular box or roll of photographic material. They do not represent standards or specifications that must be met by Carestream Health, Inc. The company reserves the right to change and improve product characteristics at any time.

Automatic Processing Recommendations: In general, processing is recommended in X-OMAT and RP X-OMAT Processors using RP X-OMAT Developer and Replenisher and RP X-OMAT LO Fixer and Replenisher.		Replenishment Rate Recommendations for X-OMAT or RP X-OMAT Processors (Replenishment by length)				
Recommended Starter Volumes		Film Size Processed	Use Condition	Average Number of Films per 8 hours processor operation	Replenishment Rates (ml per 35 x 43 cm)	
Developer	Starter (Added to processor developer tank)				Developer	Fixer
RP	89 ml (3 fl. Oz.) per 3.78 Litres (1 gallon)	35 x 35 cm (only)	High Medium Low	90 sheets or more 30 – 90 sheets 30 sheets or less*	50 65 80	70 85 100
		Average size intermix	High Medium Low	115 sheets or more 40 – 115 sheets 40 sheets or less*	50 65 80	70 85 100
		35 x 43 cm (only)	High Medium Low	75 sheets or more 25 – 75 sheets 25 sheets or less*	60 80 100	85 100 120
		*If sensitometry does not stay within control limits, flooded replenishment is recommended.				
		Please refer to Service Bulletin No. 30, available on the Carestream website or upon request, for additional processing recommendations.				

Influence of developer temperature in case of manual processing


The developing time must be adjusted as per the following table:

Temperature °C:	20	22	24.5	26.5
Developer Time (minutes)	8	7	5	4

Storage and Handling

Storage -

Unexposed:



10–24 °C (50–75 °F)

Do not refrigerate or freeze as this can cause condensation to occur.



30–50 %RH



Protect from heat and radioactive sources. Film is to be properly shielded from x-rays, gamma rays, or penetrating radiation.

Exposed: Keep cool, dry, and properly shielded from penetrating radiation. Process as soon as possible.

Processed: 16–27 °C (60–80 °F), 30–50 %RH

The film should be used before the expiration date  indicated on the box with the lot number **LOT**.

Handling -

Hands must be clean, dry and free of lotions, etc. Film should be handled carefully by the edges to avoid physical strains such as pressure, creasing, or buckling. Luminous watches, cell phone and darkroom light leaks should be avoided.



Do not re-use. Film is a single use medical device.

Safelight Filter




Use a Ruby Red Safelight Filter, such as GBX-2, with a frosted 15-watt bulb or a LED Safelight located at least 1.22 metres (48 inches) from the film.

Latensification: Safelight exposure after primary x-ray exposure.

Hypersensitization: Safelight exposure prior to primary x-ray exposure.

Oncology EC Film

GBX-2 Safelight Filter, 15-watt bulb / 1.22 metres (48 inches)
RP X-OMAT Processor, Model M6, RP X-OMAT Chemicals, 35 °C (95 °F)

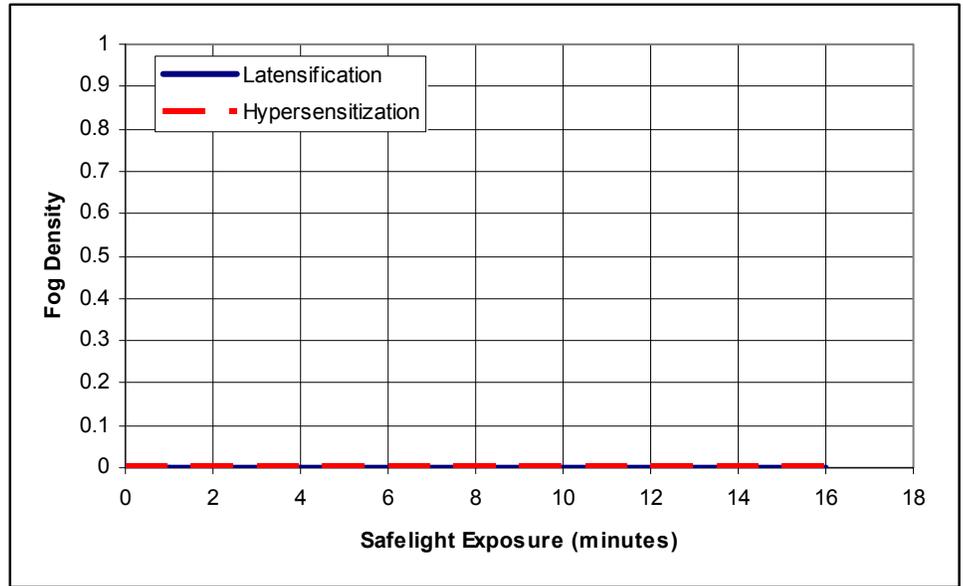

The contents of this publication are subject to change without notice.



Carestream Health France
1, rue Galilée
93192 NOISY-LE-GRAND CEDEX
FRANCE

© Carestream Health, Inc., 2017. CARESTREAM and X-OMAT are trademarks of Carestream Health.

Carestream Health, Inc. – 150 Verona Street – Rochester, NY, USA 14608

©Carestream Health, Inc. 2017, Publication No. CHSP-8604, rev. 3